

# Quick Reference Card



## GeneAtlas® IVT and WT Array Strips Fluidics Station Tray Filling Guide

### Step 1

Pipette the appropriate reagents into the consumables as shown in the bottom image. Be careful not to introduce any bubbles during that process.

### Step 2

Load the consumables into the Fluidics Station as shown in the image on the right.

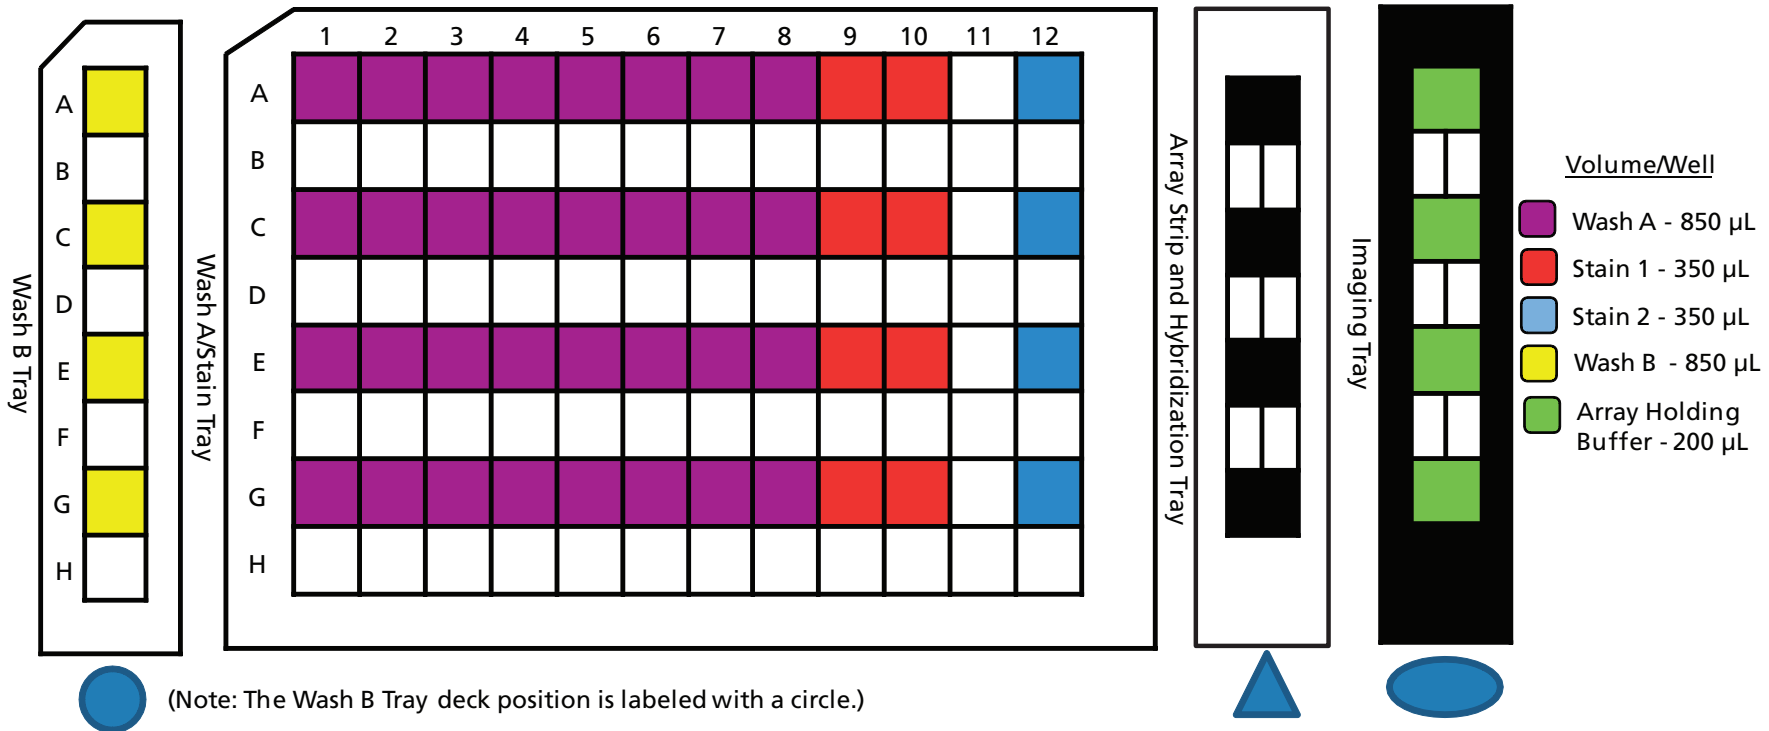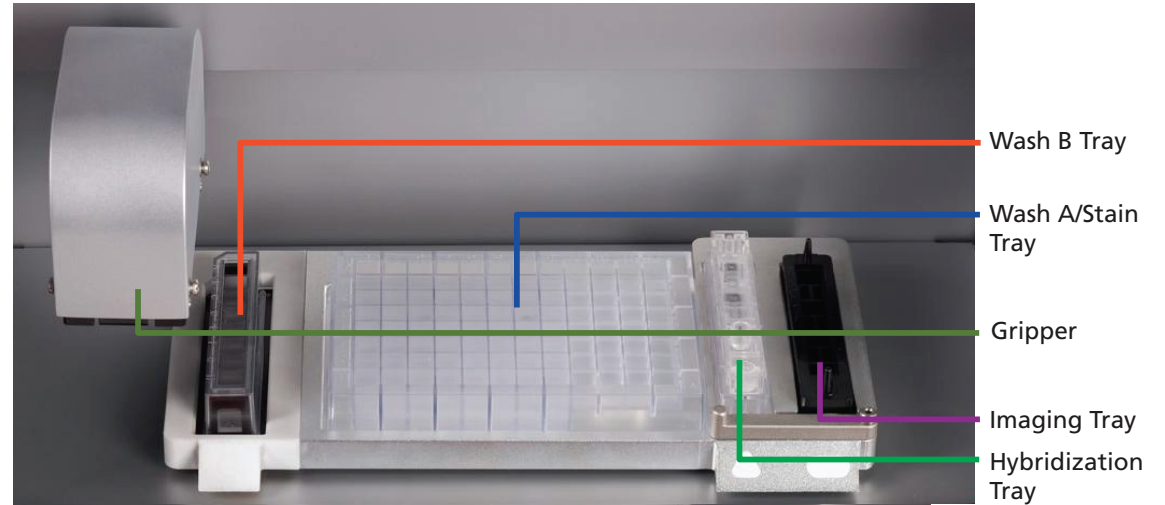

For Research Use Only. Not for use in Diagnostic Procedures.